

METHODS

METHOD OF LOCAL APPLICATION OF FOCUSED ULTRASOUND TO DEEP BRAIN STRUCTURES OF AN UNRESTRAINED UNANESTHETIZED ANIMAL

O. S. Adrianov, N. I. Vykhodtseva,
V. F. Fokin, and V. M. Avirom

UDC 616.831-008.65-031.84-092.9-02:615.837.3

KEY WORDS: focused ultrasound, optic tract, evoked potentials.

To study structural-functional relations in the CNS a widely used method is that based on blocking brain structures by exposure to various factors: electric, temperature, chemical, and so on. Changes in the animal's responses after blocking of brain structures are then studied. However, the use of all known blocking procedures is accompanied by unavoidable damage to brain structures located above the blocked formation, and in addition, the operations are complicated by secondary phenomena in neighboring structures as a result of disturbance of the circulation in part of the vascular system. The method based on application of focused ultrasound (FUS) to block deep brain structures is known to be free from the above drawbacks [1, 2].

However, with the technique described previously it is impossible to induce such a block in an unrestrained animal, because the experimental procedure of application of FUS to deep brain structures requires fixation of the animal in a stereotaxic apparatus, to which the ultrasonic generator is rigidly connected. The animal must therefore be immobilized or anesthetized.

The aim of this investigation was to devise a method of studying functional changes after blocking of CNS structures through application of FUS in the course of performance of a behavioral act by the animal. The result of ultrasonic application was assessed by studying changes in electrical activity (evoked potential - EP) of the optic tract.

EXPERIMENTAL METHOD

In the method developed, the fixing device with the ultrasonic generator is oriented in accordance with the coordinates of the structure to be blocked and is implanted on the animal's skull, and ultrasound is applied during performance of a behavioral act by the animal. This device has a body consisting of a hollow cylinder, whose internal diameter corresponds to the external diameter of the ultrasonic radiator, and is filled with sound-conducting fluid, and a miniature piezoceramic ultrasonic radiator, shaped like the segment of a sphere 1.8 cm in diameter with focal distance of 2.5 cm, and a working frequency of 0.975 MHz (Fig. 1). To implant the apparatus, the head of the previously anesthetized animal was fixed in the halter of a stereotaxic apparatus. A midline skin incision was made, the muscles dissected, and the part of the cranial bone above the structure to be irradiated was exposed. Using the indicator of the micromanipulator of the stereotaxic instrument, a point on the cranial bone located above the center of the area to be blocked was determined. A circle with its center as its point, and with a diameter equal to that of the radiator, was marked out on the animal's skull. A burr-hole of this diameter was then drilled. The body of the instrument was placed above the burr-hole and fixed to the skull with screws. The airtightness of fitting of the apparatus was ensured by the use of self-hardening plastic of the "Stirakril" type.

The effect of blocking and the course of adaptation were monitored by recording electrophysiological parameters through implanted electrodes: cortical (a silver wire 0.3 mm in diameter insulated with varnish) and subcortical, bipolar (nichrome wire 0.1 mm in diameter insulated with varnish).

Brain Research Institute, All-Union Mental Health Scientific Center, Academy of Medical Sciences of the USSR, Moscow. Translated from *Byulleten' Éksperimental'noi Biologii i Meditsiny*, Vol. 98, No. 7, pp. 115-117, July, 1984. Original article submitted July 21, 1983.

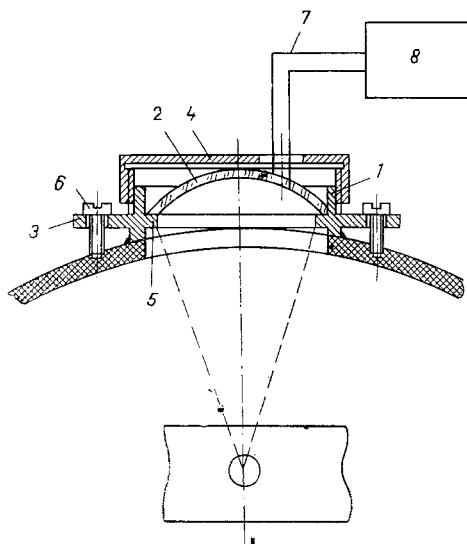


Fig. 1

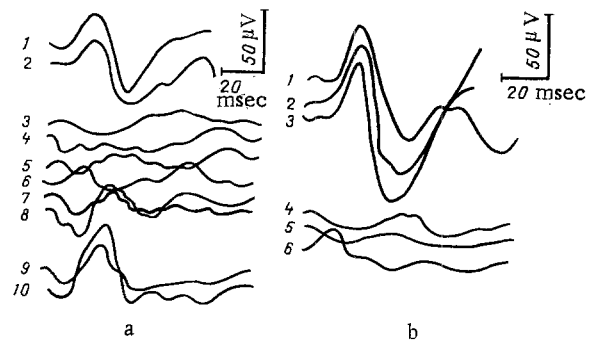


Fig. 2

Fig. 1. Diagram of apparatus for local application of FUS to brain structures of an unrestrained animal. 1) Body, 2) focusing radiator, 3) device for fixing body to animal's skull, 4) tight-fitting lid, 5) flange of body, 6) screws, 7) flexible cable, 8) ultrasonic generator.

Fig. 2. Reversible (a) and irreversible (b) changes in evoked potentials of optic tract before and after application of FUS (continuous irradiation). Explanation in text.

The period of adaptation during which the normal brain activity of the animal was restored to its preoperative level (the amplitude of the EEG reached 20-30 μ V, a desynchronization reaction was observed during 5-10% of the recording time, and the level of correct conditioned-reflex responses was 85%) as a rule lasted 3 days. The animal was then placed in an experimental chamber, the tight-fitting lid was removed, and the body filled with degassed physiological saline, warmed to 37°C. The focusing radiator, connected by a flexible cable to the ultrasonic generator, was placed inside the body (Fig. 1). The electrodes were connected through a plug and socket with a flexible cable to the input of a biopotential amplifier or electroencephalograph.

EXPERIMENTAL RESULTS

The possibility of reversible blocking of the optic tract by the use of continuous application of ultrasound was studied. With an intensity of ultrasound of 63 W/cm² and a duration of application of 30 sec, a reversible blocking effect was obtained, consisting of initial depression and subsequent restoration of EP. The presence of this effect is illustrated by Fig. 2a, in which traces of biopotentials 1 and 2 were obtained before application of ultrasound, and traces 3-8 at various times after application. Traces 9 and 10 were obtained 30 min after ultrasonic irradiation. Depression of all phases of EP will be noted. The shape of the EP was gradually restored 15 min after the end of irradiation, and in the initial stage of recovery the amplitude of the first stage of EP was higher than normal, whereas the amplitude of the second phase remained unchanged, although its latent period was appreciably lengthened. Recovery of all phases of EP was observed in this case after a few tens of minutes.

If the duration of ultrasonic irradiation was increased to 60 sec, irreversible blocking of conduction of excitation, accompanied by irreversible damage to brain tissue was observed. Disappearance of all phases of EP after irradiation can be seen in Fig. 2b: Traces 1-3 were obtained before application of ultrasound, traces 4-6 a few hours after ultrasonic irradiation.

The method described above can thus be used to study the dynamics of the phases of behavior during the first minutes of blocking of particular brain structures while the animal is performing a behavioral act; in this way additional reliable information can be obtained on the character of functioning of brain structures and on the localization of cerebral functions.